Apollo Dental Products by MIDMARK®

Maintenance Schedule

Scroll Air Compressor

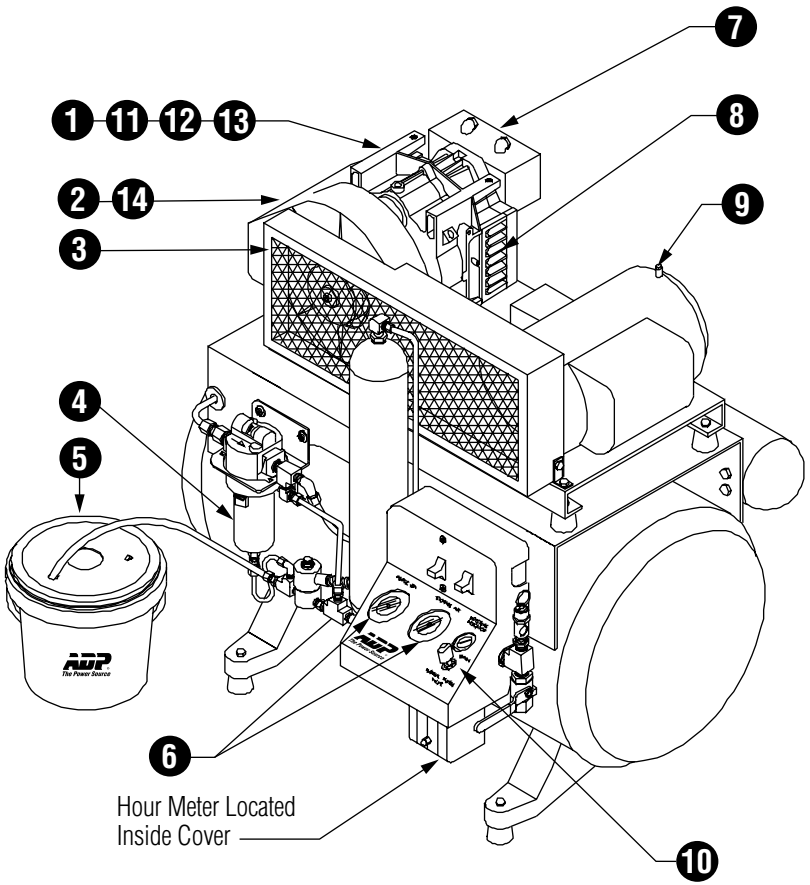

ITEM	INSPECTION	SCHEDULE CALENDAR Weekly	Monthly	Annually
Moisture Indicator **#10**	Confirm Blue	I		
Condensate Drain **#5**	Empty As Needed	I		
Pump-Up Time **#6**	Confirm Time (35-40 Sec.)		I	
Ultrair Element **#4**	Replace If Red		I	R

		SCHEDULE HOURS 500	2,500	5,000	10,000	20,000
Intake Filter **#7**	Clean/Replace	I	R			
Blower Fan **#2**	Clean			I		
Fan Duct **#14**	Clean			I		
Compressor Fins **#8**	Clean			I		
Compressor **#1**	Grease			R		
Motor **#9**	Grease			R		
Tip Seal **#11**	Replace				R	
Dust Seal **#12**	Replace		I		R	
V-Belt **#3**	Inspect/Replace	**Readjust**	I		R	
Compressor **#13**	Overhaul (Consult ADP)				I	R Consult ADP

I = Inspection R = Replace

SERVICE & MAINTENANCE LOG

	Service Performed:	Date:	Serviced By:
1.			
2.			
3.			
4.			
5.			
6.			

Apollo Dental Products, Inc.
245 W. Dakota Ave. • Clovis, California 93612 • (559) 292-1444 • (800) 233-4151 • Fax (559) 292-1555 • Fax (800) 880-9412 • E-Mail: support@apollodental.com • www.apollodental.com

AMI60317 Rev. 1/01